

Hollister Sterile Leg Bags Flip Tap



Guide for Use

Applying the bag


Single patient use only.

Ensure these simple instructions are followed for maximum comfort and security.

Remove bag from packaging by peeling from upper right-hand corner. Close drain tap before connecting. Connect the stepped mount connector to the catheter or sheath. Firmly fix to thigh or calf with straps or holster.

Applying the leg bag straps


Adjust the straps so they are comfortable and secure.



Precautions

- To ensure adequate circulation, do not overtighten.
- Check the area under the straps regularly for skin irritation or trauma.
- To prevent improper drainage do not attach leg bag to knee.


Holster fixation (holster not included)

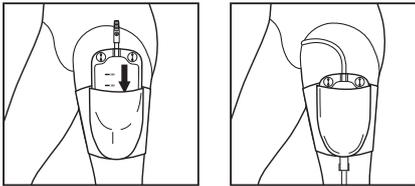


Draining leg bag

Tap closed

Tap open

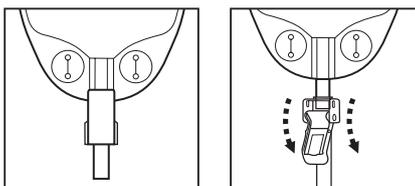

Connecting to a night drainage bag (not included) for extra capacity

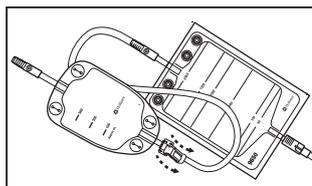

To remove and dispose

(Please follow all local disposal regulations)

Remove leg bag straps.

Warnings

- Disinfection and sterilisation may compromise the product. This may result in odour or leakage.

Precautions

 Single patient – multiple use. Sharing this product with multiple users creates a risk of infection.

Between uses, empty and rinse leg bag with lukewarm water or clean per healthcare professional recommendations. Hang to dry away from heat. Wipe outside of bag and tubing with damp cloth as needed. Clean the connector with an alcohol wipe before each use.

Notes

Contact a healthcare professional for help with continence care products. In case of serious injury (incident) in relation to your use of the product, please contact your local distributor or manufacturer and your local competent authority. For more information, see www.hollister.com/authority or contact your local distributor.

<ul style="list-style-type: none"> • Urinary leg bag with drain valve and attached tubing • Urinary leg bag straps 	<ul style="list-style-type: none"> • Stepped mount connectors 
--	--

-  Hand wash
-  Drip dry
-  Do not iron
-  Do not bleach
-  Do not dry clean

Discard when visibly damaged or stained.

 Not made with natural rubber latex

Prior to use, be sure to read the Instructions for Use for information regarding Intended Use, Contraindications, Warnings, Precautions and Instructions.

Product Ordering Codes – Sterile

9621K – 500ml / 10cm inlet

9631K* – 800ml / 10cm inlet

9624K – 500ml / 50cm inlet

9632K – 800ml / 50cm inlet

*Not available in New Zealand

Hollister Non-Sterile Leg Bags Flip Tap




Guide for Use

Applying the leg bag


Ensure the drain tap is closed.

1. To shorten the inlet tubing of the leg bag (if desired) cut the tubing.
2. Insert the stepped mount connector if present then attach to the sheath (catheter). Make sure tubing is not kinked or obstructed.

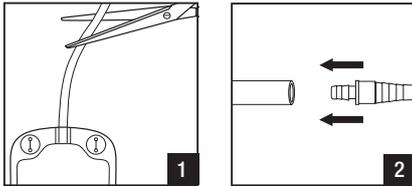

Applying the leg bag straps

Adjust the straps so they are comfortable and secure.




Precautions


- To ensure adequate circulation, do not overtighten.
- Check the area under the straps regularly for skin irritation or trauma.
- To prevent improper drainage do not attach leg bag to knee.

Draining leg bag


Tap closed



Tap open



Connecting to a night drainage bag (not included) for extra capacity

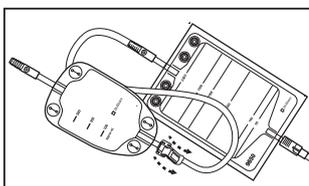

For more information or samples please call:

AU Customer Care **1800 880 851**
www.hollister.com.au

NZ Customer Service **0800 678 669**
www.hollister.co.nz

To remove and dispose

(Please follow all local disposal regulations)

Remove leg bag straps.

Warnings

- Disinfection and sterilisation may compromise the product. This may result in odour or leakage.

Precautions

 Single patient – multiple use. Sharing this product with multiple users creates a risk of infection.

Between uses, empty and rinse leg bag with lukewarm water or clean per healthcare professional recommendations. Hang to dry away from heat. Wipe outside of bag and tubing with damp cloth as needed. Clean the connector with an alcohol wipe before each use.

Notes

Contact a healthcare professional for help with continence care products. In case of serious injury (incident) in relation to your use of the product, please contact your local distributor or manufacturer and your local competent authority. For more information, see www.hollister.com/authority or contact your local distributor.

<ul style="list-style-type: none"> • Urinary leg bag with drain valve and attached tubing • Urinary leg bag straps 	<ul style="list-style-type: none"> • Stepped mount connectors 
--	--



Hand wash



Drip dry



Do not iron



Do not bleach



Do not dry clean

Discard when visibly damaged or stained.

Prior to use, be sure to read the Instructions for Use for information regarding Intended Use, Contraindications, Warnings, Precautions and Instructions.

Product Ordering Codes – Non-Sterile

9652 – 500ml / 50cm inlet

9653 – 800ml / 50cm inlet